

धात्विक चूर्ण — अंशशोधित फनल द्वारा  
प्रवाह (गुस्तावस्सों प्रवाहमीटर) दर ज्ञात  
करना

( पहला पुनरीक्षण )

**Metallic Powders — Determination of  
Flow Rate by Means of a Calibrated  
Funnel (Gustavsson Flowmeter)**

( *First Revision* )

ICS 77.160

© BIS 2023

© ISO 2020



भारतीय मानक ब्यूरो  
BUREAU OF INDIAN STANDARDS  
मानक भवन, 9 बहादुर शाह ज़फर मार्ग, नई दिल्ली - 110002  
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG  
NEW DELHI - 110002

[www.bis.gov.in](http://www.bis.gov.in) [www.standardsbis.in](http://www.standardsbis.in)

## NATIONAL FOREWORD

This Indian Standard (First Revision) which is identical to ISO 13517 : 2020 'Metallic powders — Determination of flow rate by means of a calibrated funnel (Gustavsson flowmeter)' issued by the International Organization for Standardization (ISO), was adopted by the Bureau of Indian Standards on the recommendation of the Powder Metallurgical Materials and Products Sectional Committee and approval of the Metallurgical Engineering Division Council.

This standard was first published in 2019. The first revision of this standard has been undertaken to align with the latest version ISO 13517 : 2020 under dual numbering system to harmonize it with the latest developments that have taken place at international level.

Major changes compared to the previous version are:

- a) Tolerance for the funnel angle has been added;
- b) Reference grit has been used instead of chinese emery grit; and
- c) The mandatory clauses **2** and **3** (normative references and terms and definitions) have been added and the subsequent clauses have been renumbered.

The text of ISO standard has been approved as suitable for publication as an Indian Standard without deviations. Certain terminologies and conventions are, however, not identical with those used in Indian Standard. Attention is especially drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, it should be read as 'Indian Standard'
- b) Comma (,) has been used as a decimal marker while in Indian Standards the current practice is to use a point (.) as the decimal marker.

In reporting the result of a test or analysis made in accordance with this standard, if the final value, observed or calculated, is to be rounded off, it shall be done in accordance with IS 2 : 2022 'Rules for rounding off numerical values (*second revision*)'.

# Contents

Page

<b>1</b>	<b>Scope</b> .....	<b>1</b>
<b>2</b>	<b>Normative references</b> .....	<b>1</b>
<b>3</b>	<b>Terms and definitions</b> .....	<b>1</b>
<b>4</b>	<b>Principle</b> .....	<b>1</b>
<b>5</b>	<b>Apparatus</b> .....	<b>1</b>
<b>6</b>	<b>Calibration of the funnel</b> .....	<b>3</b>
	6.1 Calibration by the manufacturer of the funnel.....	3
	6.2 Calibration by the user of the funnel.....	3
<b>7</b>	<b>Sampling</b> .....	<b>3</b>
<b>8</b>	<b>Procedure</b> .....	<b>4</b>
<b>9</b>	<b>Expression of results</b> .....	<b>4</b>
<b>10</b>	<b>Precision</b> .....	<b>4</b>
<b>11</b>	<b>Test report</b> .....	<b>5</b>
	<b>Bibliography</b> .....	<b>6</b>



*Indian Standard*

METALLIC POWDERS — DETERMINATION OF FLOW RATE BY  
MEANS OF A CALIBRATED FUNNEL (GUSTAVSSON  
FLOWMETER)  
( *First Revision* )

## 1 Scope

This document specifies a method for determining the flow rate of metallic powders, including powders for hardmetals and mixes of metallic powders and organic additives such as lubricants, by means of a calibrated funnel (Gustavsson flowmeter).

The method is applicable only to powders which flow freely through the specified test orifice.

## 2 Normative references

There are no normative references in this document.

## 3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

## 4 Principle

Measurement of the time required for 50 g of a metallic powder to flow through the orifice of a calibrated funnel of standardized dimensions.

## 5 Apparatus

**5.1 Calibrated funnel**, with the dimensions shown in [Figure 1](#) (see [Clause 6](#)). The dimensions shown for the flowmeter funnel, including the orifice, are not to be considered controlling factors. Calibration with reference grit, as specified in [Clause 6](#), determines the working flow rate of the funnel.

The funnel shall be made of a non-magnetic, corrosion-resistant metallic material with sufficient wall thickness and hardness to withstand distortion and excessive wear.

**5.2 Stand and horizontal vibration-free base**, to support the funnel rigidly, e.g. as indicated in [Figure 2](#).

**5.3 Balance**, of sufficient capacity, capable of weighing the test portion to an accuracy of  $\pm 0,05$  g.


**5.4 Timing device**, capable of measuring the elapsed time to an accuracy of  $\pm 0,1$  s.

**5.5 Reference grit**, a reference powder used for calibration of the funnel<sup>1)</sup>.

---


1) Material complying with [5.5](#) can be purchased as “Chinese emery grit”. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the company named above. Equivalent products may be used if they can be shown to lead to the same results.

Dimensions in millimetres

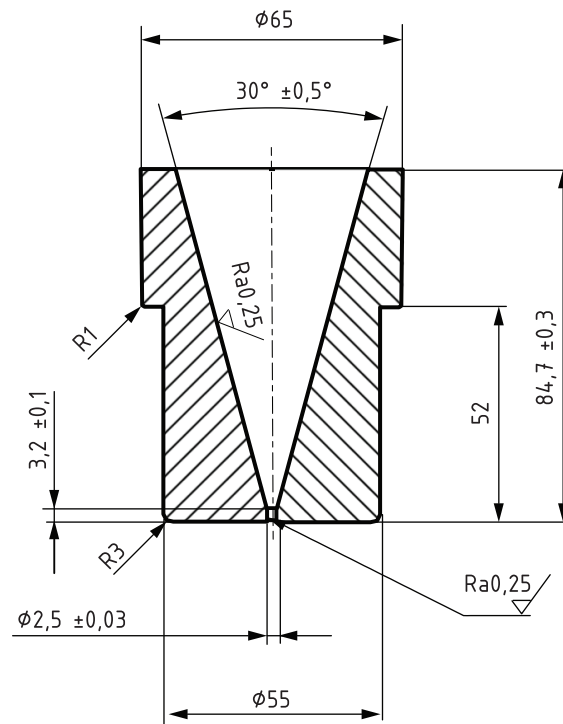

NOTE For dimensions with no individual tolerance, refer to ISO 2768-1 and tolerance class medium. Applicable only for new funnels.

**Figure 1 — Calibrated funnel (Gustavsson flowmeter)**

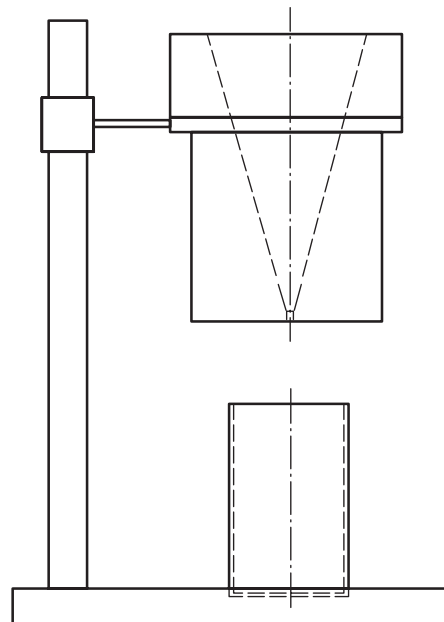

**Figure 2 — Arrangement of calibrated funnel and stand**

## 6 Calibration of the funnel

### 6.1 Calibration by the manufacturer of the funnel

The manufacturer shall supply the flowmeter calibrated as follows.

- a) Dry the reference grit (5.5) in an open and clean glass jar at 110 °C for 60 min in air.
- b) Cool the reference grit to room temperature in a desiccator.
- c) Weigh out 50,0 g  $\pm$  0,1 g of the grit.
- d) Follow the procedure outlined in [Clause 8](#).
- e) Repeat the procedure with the same 50 g mass of the grit, until there are five determinations within 0,4 s;
- f) The average of these five determinations is stamped on the bottom of the funnel and shall be within 40,0 s  $\pm$  0,5 s.

### 6.2 Calibration by the user of the funnel

The flow rate of the reference sample shall be determined by the above method. If the flow rate has changed to be outside 40,0 s/50 g  $\pm$  0,5 s/50 g, a correction factor shall be used when measuring different powders. This correction factor is obtained by dividing 40,0 by this new value for the Reference grit.

It is recommended that the users periodically verify whether a correction is needed or not.

It is recommended that, before a correction factor is adopted, the cause of the change be investigated. If the flow rate has decreased, it is probable that repeated use has burnished the orifice and a (new) correction factor is justified. An increase in flow rate may indicate a coating of soft powder on the orifice. This coating should be carefully removed and the calibration test repeated.

It is recommended that the use of a funnel be discontinued after the duration of flow of the reference sample has decreased to less than 37 s.

## 7 Sampling

7.1 The mass of the test sample shall be at least 200 g.

7.2 In general, the powder shall be tested in the as-received condition. In certain cases, and after agreement between the supplier and user, the powder may be dried. However, if the powder is susceptible to oxidation, the drying shall take place in a vacuum or in inert gas. If the powder contains volatile substances, it shall not be dried.

7.3 Immediately before the test, weigh out a 50,0 g  $\pm$  0,1 g test portion.

7.4 Alternatively, a test portion of 90 g to 110 g can be sampled and weighed to a precision of  $\pm$  0,1 g or better.

NOTE The intention of the alternative execution is to facilitate full automation of measurement of flow and apparent density of powders.

7.5 The determination shall be carried out on three test portions.

## 8 Procedure

Transfer the test portion to the funnel, keeping the discharge orifice closed by a dry finger. Take care that the stem of the funnel is filled with powder. Start the timing device (5.4) when the orifice is opened and stop it at the instant when the last of the powder leaves the orifice. Record the elapsed time measured to the nearest 0,1 s.

Alternatively, the orifice can be kept open, when the test portion is transferred to the funnel with the rest of the procedure being the same.

If the powder does not begin to flow when the orifice is opened, one slight tap on the funnel to start the flow is permitted. If this has no effect, or if the flow stops during the test, the powder is considered to possess no flowability according to the test method described in this document.

## 9 Expression of results

Calculate the arithmetic mean of the results of the three determinations and report the value in seconds per 50 g, rounded to the nearest second.

If the alternative size of the test portion according to 7.4 is applied, the result of each determination shall, before the calculation of the arithmetic mean of the results, be divided by the mass of the sample and then be multiplied by 50 g. The result is thus recalculated in seconds per 50 g.

If a correction factor (see 6.2) should be used, the average shall be multiplied by this correction factor.

## 10 Precision

Two plain iron powders and four iron or bronze powder mixes were included in the inter-laboratory study to develop this precision statement. Compositions of the mixes are presented in Table 1.

**Table 1 — Mix compositions of powder included in the inter-laboratory study**

Designation	Mix composition
Plain iron powder 1	Plain atomized iron powder
Plain iron powder 2	Plain sponge iron powder
Bronze powder mix	Bronze powder + 0,375 % Stearic acid + 0,375 % Zinc stearate
Iron powder mix 1	Atomized iron powder + 0,8 % Graphite + 0,8 % Amide wax
Iron powder mix 2	Atomized iron powder + 2 % Ni powder + 0,8 % Graphite + 0,8 % Amide wax
Iron powder mix 3	Atomized iron powder + 0,8 % Graphite + 0,8 % Zinc stearate

In Table 2, the repeatability and reproducibility are presented as one standard deviation.

**Table 2 — Repeatability and reproducibility as standard deviations**

Tested powder	Level (average flow time)	Repeatability standard deviation	Reproducibility standard deviation
		$s_r$	$s_R$
Plain iron powder 1	25 s	0,3 s	0,6 s
Plain iron powder 2	32 s	0,5 s	0,7 s
Bronze powder mix	45 s	2,6 s	3,2 s
Iron powder mix 1	48 s	1,1 s	2,2 s
Iron powder mix 2	56 s	1,0 s	2,0 s
Iron powder mix 3	60 s	0,8 s	4,7 s



The difference between two test results found on identical test material by one operator using the same apparatus within the shortest feasible time interval will exceed the repeatability limit ( $r$ ), see [Table 3](#), on average not more than once in 20 cases in the normal and correct operation of the method.

Test results on identical test material reported by two laboratories will differ by more than the reproducibility limit ( $R$ ), see [Table 3](#), on average not more than once in 20 cases in the normal and correct operation of the method.

**Table 3 — Repeatability and reproducibility, difference between two tests at 95 % probability level**

Tested powder	Level (average flow time)	Repeatability limit $r$	Reproducibility limit $R$
Plain iron powder 1	25 s	0,9 s	1,8 s
Plain iron powder 2	32 s	1,3 s	2,0 s
Bronze powder mix	45 s	7,3 s	9,0 s
Iron powder mix 1	48 s	3,0 s	6,2 s
Iron powder mix 2	56 s	2,7 s	5,7 s
Iron powder mix 3	60 s	2,2 s	13,1 s

The accuracy data were determined from an experiment organized and analysed in accordance with ISO 5725-2 in 2011, involving 17 laboratories and 6 levels. Data from none of the laboratories contained outliers.

## 11 Test report

The test report shall include at least the following information:

- a) a reference to this document, i.e. ISO 13517:2020;
- b) all details for identification of the test sample;
- c) the result obtained expressed in s/50 g;
- d) the use of an open orifice;
- e) all operations not specified by this document, or regarded as optional (e.g. the drying procedure applied and whether flow has been induced by tapping the funnel);
- f) details of any occurrence which may have affected the result.

## Bibliography

- [1] ISO 2768-1, *General tolerances — Part 1: Tolerances for linear and angular dimensions without individual tolerance indications*
- [2] ISO 5725-2, *Accuracy (trueness and precision) of measurement methods and results — Part 2: Basic method for the determination of repeatability and reproducibility of a standard measurement method*



## Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 2016* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

### Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in the course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Head (Publication & Sales), BIS.

### Review of Indian Standards

Amendments are issued to standards as the need arises on the basis of comments. Standards are also reviewed periodically; a standard along with amendments is reaffirmed when such review indicates that no changes are needed; if the review indicates that changes are needed, it is taken up for revision. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition by referring to the website-[www.bis.gov.in](http://www.bis.gov.in) or [www.standardsbis.in](http://www.standardsbis.in).

This Indian Standard has been developed from Doc No.: MTD 25 (20388).

### Amendments Issued Since Publication

Amend No.	Date of Issue	Text Affected

## BUREAU OF INDIAN STANDARDS

### Headquarters:

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110002

Telephones: 2323 0131, 2323 3375, 2323 9402

Website: [www.bis.gov.in](http://www.bis.gov.in)

### Regional Offices:

	Telephones
Central : 601/A, Konnectus Tower -1, 6 <sup>th</sup> Floor, DMRC Building, Bhavbhuti Marg, New Delhi 110002	{ 2323 7617
Eastern : 8 <sup>th</sup> Floor, Plot No 7/7 & 7/8, CP Block, Sector V, Salt Lake, Kolkata, West Bengal 700091	{ 2367 0012 2320 9474
Northern : Plot No. 4-A, Sector 27-B, Madhya Marg, Chandigarh 160019	{ 265 9930
Southern : C.I.T. Campus, IV Cross Road, Taramani, Chennai 600113	{ 2254 1442 2254 1216
Western : Plot No. E-9, Road No.-8, MIDC, Andheri (East), Mumbai 400093	{ 2821 8093

**Branches :** AHMEDABAD. BENGALURU. BHOPAL. BHUBANESHWAR. CHANDIGARH. CHENNAI. COIMBATORE. DEHRADUN. DELHI. FARIDABAD. GHAZIABAD. GUWAHATI. HIMACHAL PRADESH. HUBLI. HYDERABAD. JAIPUR. JAMMU & KASHMIR. JAMSHEDPUR. KOCHI. KOLKATA. LUCKNOW. MADURAI. MUMBAI. NAGPUR. NOIDA. PANIPAT. PATNA. PUNE. RAIPUR. RAJKOT. SURAT. VISAKHAPATNAM.