

---

---

**Plastics — Determination of the  
viscosity of polymers in dilute solution  
using capillary viscometers —**

Part 1:  
**General principles**

*Plastiques — Détermination de la viscosité des polymères en solution  
diluée à l'aide de viscosimètres à capillaires —*

*Partie 1: Principes généraux*





**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
3.1 Terms related to any liquid.....	1
3.2 Terms related to polymer solutions.....	2
<b>4 Principle</b> .....	<b>4</b>
<b>5 Apparatus</b> .....	<b>5</b>
<b>6 Solutions</b> .....	<b>8</b>
6.1 Preparation.....	8
6.2 Concentration.....	9
<b>7 Temperature of measurement</b> .....	<b>9</b>
<b>8 Procedure</b> .....	<b>9</b>
8.1 General.....	9
8.2 Preparing and charging the viscometer.....	9
8.3 Efflux time measurement.....	10
<b>9 Expression of results</b> .....	<b>10</b>
9.1 Reduced viscosity and intrinsic viscosity.....	10
9.2 <i>K</i> -value.....	11
<b>10 Test report</b> .....	<b>11</b>
<b>Annex A (normative) Cleaning of apparatus</b> .....	<b>12</b>
<b>Annex B (informative) Notes on sources of error</b> .....	<b>13</b>
<b>Bibliography</b> .....	<b>16</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 249, *Plastics*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This fourth edition cancels and replaces the third edition (ISO 1628-1:2009), which has been technically revised. It also incorporates the Amendment 1 ISO 1628-1:2009/Amd 1:2012.

The main changes compared to the previous edition are as follows:

- ISO 3205 (withdrawn) has been deleted from [Clause 2](#);
- the figure keys have been revised;
- nominal viscometer constant has been added to [Table 1](#);

A list of all parts in the ISO 1628 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

# Plastics — Determination of the viscosity of polymers in dilute solution using capillary viscometers —

## Part 1: General principles

### 1 Scope

This document defines the general conditions for the determination of the reduced viscosity, intrinsic viscosity and *K*-value of organic polymers in dilute solution. It defines the standard parameters that are applied to viscosity measurement.

This document is used to develop standards for measuring the viscosities in solution of individual types of polymer. It is also used to measure and report the viscosities of polymers in solution for which no separate standards exist.

### 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3105, *Glass capillary kinematic viscometers — Specifications and operating instructions*

ISO 80000-1, *Quantities and units — Part 1: General*

ISO 80000-4, *Quantities and units — Part 4: Mechanics*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 80000-1, ISO 80000-4 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

#### 3.1 Terms related to any liquid

##### 3.1.1

##### **viscosity**

property of a fluid sheared between two parallel plates, one of which moves relative to the other in uniform rectilinear motion in its own plane, defined by the Newton formula

$$\tau = \eta \dot{\gamma}$$

where

$\tau$  is the shear stress;

$\eta$  is the viscosity;

$\dot{\gamma}$  is the velocity gradient or rate of shear, given by  $\frac{dV}{dz}$  where  $V$  is the velocity of one plane relative to the other and  $z$  the coordinate perpendicular to the two planes.

Note 1 to entry: The dimensions of viscosity are  $ML^{-1}T^{-1}$ .

Note 2 to entry: The units of viscosity are Pa·s.

Note 3 to entry: For practical use, the sub-multiple  $10^{-3}$  Pa·s is more convenient.

Note 4 to entry: Viscosity is usually taken to mean “Newtonian viscosity”, in which case the ratio of shearing stress to velocity gradient is constant. In non-Newtonian behaviour, which is the usual case with high-polymer solutions, the ratio varies with the shear rate. Such ratios are often called “apparent viscosities” at the corresponding shear rate.

### 3.1.2 viscosity/density ratio kinematic viscosity

$\nu$   
ratio defined by the formula

$$\nu = \frac{\eta}{\rho}$$

where  $\rho$  is the density of the fluid at the temperature at which the viscosity is measured

Note 1 to entry: The dimensions of kinematic viscosity are  $L^2T^{-1}$ .

Note 2 to entry: The units of kinematic viscosity are  $m^2 \cdot s^{-1}$ .

Note 3 to entry: For practical use, the sub-multiple  $10^{-6} m^2 \cdot s^{-1}$ , i.e.  $mm^2 \cdot s^{-1}$ , is more convenient.

## 3.2 Terms related to polymer solutions

### 3.2.1 relative viscosity viscosity ratio

$\eta_r$   
ratio of the viscosity of the polymer solution (of stated concentration)  $\eta$  and the viscosity of the pure solvent  $\eta_0$ , at the same temperature:

$$\eta_r = \frac{\eta}{\eta_0}$$

Note 1 to entry: The ratio has no dimensions.

### 3.2.2 relative viscosity increment viscosity ratio increment and specific viscosity viscosity ratio minus one

$$\left( \frac{\eta}{\eta_0} \right) - 1 = \frac{\eta - \eta_0}{\eta_0}$$

Note 1 to entry: The increment has no dimensions.

### 3.2.3 reduced viscosity viscosity number

$I$

ratio of the relative viscosity increment to the polymer concentration  $c$  in the solution:

$$I = \frac{\eta - \eta_0}{\eta_0 c}$$

Note 1 to entry: The dimensions of reduced viscosity are  $L^3M^{-1}$ .

Note 2 to entry: The units of reduced viscosity are  $m^3/kg$ .

Note 3 to entry: For practical use, the sub-multiple  $10^{-3} m^3/kg$ , i.e.  $cm^3/g$ , is more convenient and the commonly quoted numerical values for reduced viscosity (viscosity number) use these practical units.

Note 4 to entry: The reduced viscosity is usually determined at low concentration (less than  $5 kg/m^3$ , i.e.  $0,005 g/cm^3$ ), except in the case of polymers of low molar mass, for which higher concentrations is necessary.

### 3.2.4 inherent viscosity logarithmic viscosity number

ratio of the natural logarithm of the viscosity ratio to the polymer concentration in the solution:

$$\frac{\ln\left(\frac{\eta}{\eta_0}\right)}{c}$$

Note 1 to entry: The dimensions and units are the same as those given in [3.2.3](#).

Note 2 to entry: The inherent viscosity is usually determined at low concentration (less than  $5 kg/m^3$ , i.e.  $0,005 g/cm^3$ ), except in the case of polymers of low molar mass, for which higher concentrations is necessary.

### 3.2.5 intrinsic viscosity limiting viscosity number

$[\eta]$

limiting value of the reduced viscosity or of the *inherent viscosity* ([3.2.4](#)) at infinite dilution:

$$[\eta] = \lim_{c \rightarrow 0} \left( \frac{\eta - \eta_0}{\eta_0 c} \right)$$

$$[\eta] = \lim_{c \rightarrow 0} \frac{\ln\left(\frac{\eta}{\eta_0}\right)}{c}$$

Note 1 to entry: The dimensions and units are the same as those given in [3.2.3](#).

Note 2 to entry: The effect of the shear rate on the functions defined in [3.2.1](#) to [3.2.5](#) has been neglected, since this effect is usually negligible for values of the reduced viscosity, inherent viscosity and intrinsic viscosity less than  $0,5 m^3/kg$ , i.e.  $500 cm^3/g$ . Strictly speaking, all these functions can be defined at the limiting (preferably infinitely small) value of the shear rate.

### 3.2.6 $K$ -value

constant, independent of the concentration of the polymer solution and peculiar to the polymer sample, which is a measure of the average degree of polymerization:

$$K\text{-value} = 1\ 000\ k$$

Note 1 to entry: According to H. Fikentscher<sup>[1]</sup>,  $k$  is calculated as follows:

$$\lg \eta_r = \left( \frac{75k^2}{1+150kc} + k \right) 100c$$

and therefore

$$k = \frac{1,5 \lg \eta_r - 1 + \sqrt{1 + \left( \frac{2}{c} + 2 + 1,5 \lg \eta_r \right)^2}}{150 + 300c}$$

where

$\eta_r = \frac{\eta}{\eta_0}$  is the viscosity ratio (see [3.2.1](#));

$c$  is the concentration, in  $10^3 \text{ kg/m}^3$ , i.e.  $\text{g/cm}^3$ .

Note 2 to entry: A limiting viscosity number  $[\eta]_k$  can be calculated from  $k$ :

$$[\eta]_k = 230,3(75k^2 + k)$$

#### 4 Principle

The data needed for the evaluation of the functions defined in [3.2](#) are obtained by means of a capillary-tube viscometer. The efflux times of a given volume of solvent  $t_0$  and of solution  $t$  are measured at fixed temperature and atmospheric-pressure conditions in the same viscometer. The efflux time of a liquid is related to its viscosity by the Poiseuille-Hagenbach-Couette formula as shown in [Formula \(1\)](#):

$$v = \frac{\eta}{\rho} = Ct - \left( \frac{A}{t^2} \right) \tag{1}$$

where

$v$  is the viscosity/density ratio ;

$C$  is a constant of the viscometer;

$A$  is a parameter of the kinetic-energy correction;

$\rho$  is the density of the liquid;

$t$  is the efflux time.

For the purposes of this document, the kinetic energy correction  $\left( \frac{A}{t^2} \right)$  shall be regarded as negligible when it is less than 3 % of the viscosity of the solvent. Hence, [Formula \(1\)](#) can be reduced to [Formula \(2\)](#):

$$v = \frac{\eta}{\rho} = Ct \tag{2}$$

Moreover, if the solution concentrations are limited so that the solvent density  $\rho_0$  and that of the solution  $\rho$  differ by less than 0,5 %, the viscosity ratio  $\frac{\eta}{\eta_0}$  will be given by the so-called “efflux time ratio”  $\frac{t}{t_0}$ .

The need for these constraints, and the consequences of not observing them, is described in [Annex B](#).



## 5 Apparatus


### 5.1 Capillary viscometer, of the suspended-level Ubbelohde type.

The use of a viscometer having the dimensions given in [Figure 1](#) or [Figure 2](#) is strongly recommended. Furthermore, it is strongly recommended that the size of the viscometer be chosen from among those listed in [Table 1](#). The choice is determined by the viscosity/density ratio of the solvent at the temperature of the measurement, as indicated in [Table 1](#). The next-smaller viscometer may also be used.

Other types of viscometer listed in ISO 3105 may be used, provided they give results equivalent to those given by the particular size of Ubbelohde viscometer chosen on the basis of the criteria specified in the preceding paragraph. In cases of dispute, an Ubbelohde viscometer shall be used.

With automated apparatus, fitted with special timing devices, equivalent results with larger sizes of capillary than those listed for the appropriate solvent viscosity/density ratio in [Table 1](#) can be obtained.

### 5.2 Viscometer holder, suitable to hold the viscometer firmly in the thermostatic bath ([5.3](#)) in the vertical position.

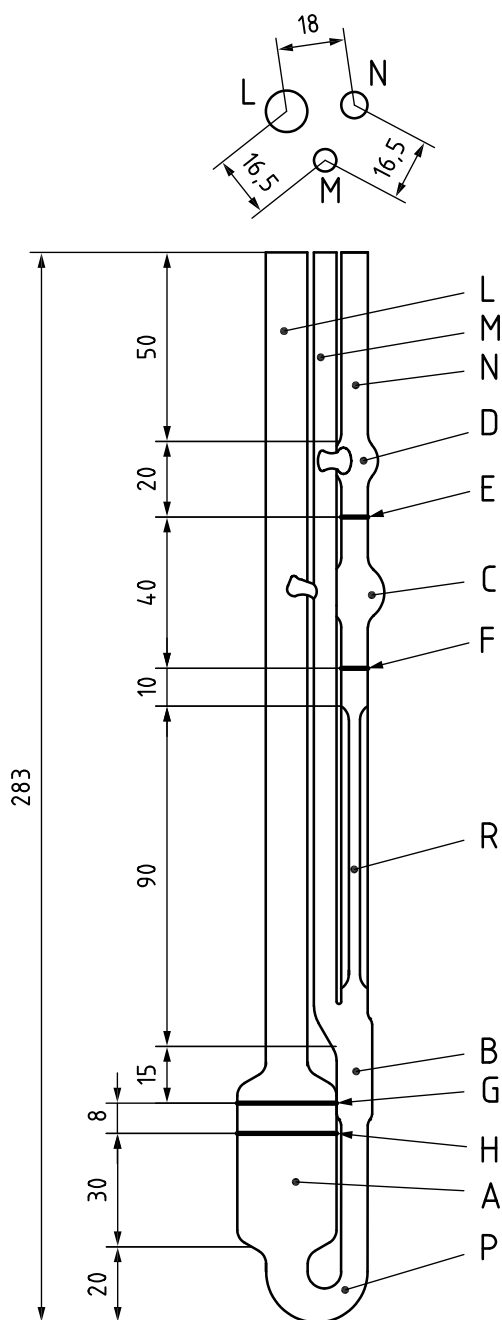

**Key**

- |         |   |   |  |
|---------|---|---|--|
| A       | lower reservoir 26 mm internal diameter | L | mounting tube 11 mm internal diameter  |
| B       | suspended level bulb                    | M | lower vent tube 6 mm internal diameter |
| C       | timing bulb                             | N | upper vent tube 7 mm internal diameter |
| D       | upper reservoir                         | P | connecting tube                        |
| E and F | timing marks                            | R | working capillary                      |
| G and H | filling marks                           |   |  |


**Figure 1 — Ubbelohde viscometer**

**5.3 Thermostatic bath**, transparent liquid or vapour bath of a size such that, during the measurement, all sections containing test liquid are at least 20 mm below the surface of the bath medium and at least 20 mm away from all boundaries of the bath tank.

The temperature control shall be such that, within the range 25 °C to 100 °C, the temperature of the bath does not vary from the specified temperature by more than 0,05 K over the length of the viscometer, or between the viscometers if several determinations are carried out simultaneously.

At temperatures higher than 100 °C, the tolerance shall be  $\pm 0,2$  °C.

Dimensions in millimetres

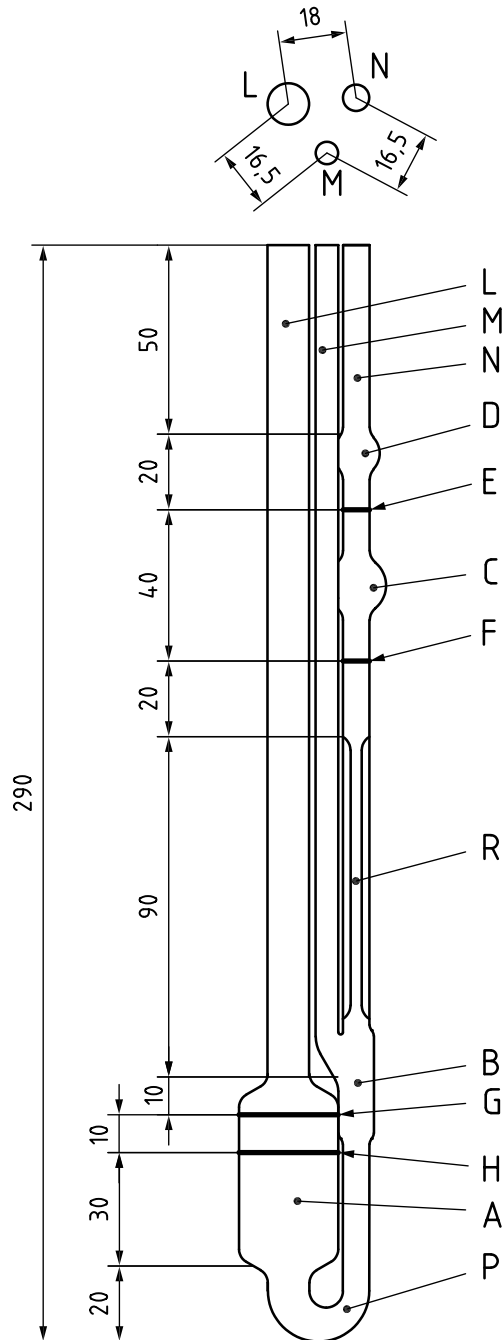

NOTE For key, see [Figure 1](#).

Figure 2 — DIN Ubbelohde viscometer

**5.4 Temperature-measuring device**, thermometer, reading to 0,02 °C in the range in which it will be used and in a known state of calibration, is suitable.

**5.5 Timing device**. Any timing device may be used providing that it can be read to 0,1 s and that its speed is constant to 0,1 % over 15 min.

**Table 1 — Ubbelohde viscometers recommended for the determination of the dilute-solution viscosity of polymers**

Viscosity/density ratio of solvent at temperature of measurement	Nominal viscometer constant	Ubbelohde conforming to ISO 3105		DIN Ubbelohde conforming to ISO 3105	
		Size No.	Inside diameter of tube R <sup>a</sup> mm	Size No.	Inside diameter of tube R <sup>a</sup> mm
mm <sup>2</sup> ·s <sup>-1</sup>	mm <sup>2</sup> ·s <sup>-2</sup>				
0,15 to 0,30	0,001	0	0,24	0	0,36
0,31 to 0,50	0,003	0C	0,36	0c	0,47
0,51 to 0,75	0,005	0B	0,46	0a	0,53
0,76 to 1,50	0,01	1	0,58	I	0,63
1,51 to 2,50	0,03	1C	0,77	Ic	0,84
2,51 to 5,00	0,05	1B	0,88	Ia	0,95
5,01 to 15,00	0,1	2	1,03	II	1,13

<sup>a</sup> The tolerance of the inside diameter of tube R is ±2 %.

## 6 Solutions

### 6.1 Preparation

The dissolution of the test sample of polymer in the solvent shall give a “true” solution, essentially free of microgels and associated macromolecules. Polymer degradation shall also be minimized. For these reasons, it is necessary for the dissolution procedure to be exactly defined and it is recommended that the following factors be specified:

- a) the solvent and its pretreatment, if any;
- b) the apparatus and the method of agitation;
- c) the temperature range within which the system is maintained during the preparation of the solution;
- d) the time interval necessary for the complete dissolution of the polymer without degradation, or at constant degradation;
- e) the stabilizer and/or the protective atmosphere used;
- f) the conditions of filtration of the solution, if applicable;
- g) visual homogeneity of the solution and expected nature/composition of the filter residue.

## 6.2 Concentration

Where no standard exists, careful consideration shall be given to the choice of solvent and the solution concentration. The solution concentration shall be chosen so that the ratio of the efflux time of the solution to the efflux time of the solvent is at least 1,2 and less than 2,0.

**NOTE** A lower limit of 1,2 ensures sufficient precision of the measured difference in efflux times. The upper limit of 2,0 prevents shear effects and non-linearity of the viscosity number in relation to concentration that can occur at higher molecular masses.

More than one concentration can therefore be used for a given polymer/solvent system, depending on the molecular mass of the polymer under test.

The concentration is preferably expressed in  $\text{kg/m}^3$  of solution or as the multiple  $10^3 \text{ kg/m}^3$ , i.e.  $\text{g/cm}^3$ .

## 7 Temperature of measurement

The temperature shall be chosen with due regard to sufficient solubility and other technical requirements, but kept constant for any particular polymer/solvent system. The temperature tolerance shall be specified. A temperature of  $25 \text{ }^\circ\text{C} \pm 0,05 \text{ }^\circ\text{C}$  shall be chosen whenever possible. If another temperature is used, use the temperature that was agreed between the parties concerned and stated in the test report.

## 8 Procedure

### 8.1 General

Measure the efflux times for the solution and the solvent successively in the same viscometer, using the procedure described in [8.2](#) and [8.3](#).

### 8.2 Preparing and charging the viscometer

**8.2.1** Maintain the bath at the specified test temperature.

**8.2.2** Charge the dry, clean viscometer (the cleaning procedure is specified in [Annex A](#)) by tilting it about  $30^\circ$  from the vertical and pouring sufficient liquid through tube L (see [Figure 1](#) or [Figure 2](#)) so that, when the viscometer is returned to the vertical, the meniscus is between the filling marks G and H. Avoid trapping air bubbles in the viscometer. The initial filling may be carried out away from the bath.

**8.2.3** Mount the viscometer in a holder in the bath, ensuring that tube N is vertical. Allow time for the charged viscometer to reach the temperature of the bath. Usually, 15 min will suffice if the measurement is to be made at  $25 \text{ }^\circ\text{C}$ . At higher temperatures, longer times is necessary. Unnecessary delays should be avoided as it is found that the most consistent results are obtained shortly after temperature equilibrium is attained with a freshly charged viscometer.

**8.2.4** This procedure shall also be followed when a measured amount of solvent is added to a solution, already contained in the viscometer, in order to create a more dilute solution for additional determinations. The additional solvent shall be maintained at the specified test temperature prior to use.

**8.2.5** In automated equipment, the viscometer is fixed in the vertical position within a temperature-controlled bath and the apparatus is designed to fill the viscometer with liquid in this position. The bath shall be maintained at the specified test temperature and an equilibration time selected in accordance with [8.2.3](#).

### 8.3 Efflux time measurement

See [Figure 1](#) or [Figure 2](#).

Close tube M and apply suction to tube N, or pressure to tube L, until the liquid reaches a level about 5 mm above mark E. Hold the liquid at this level by closing tube N.

Open tube M so that the liquid drops away from the lower end of capillary tube R.

When the liquid is clear of the end of the capillary and the lower end of tube M, open tube N. Measure the efflux time to the nearest 0,2 s as the time taken for the bottom of the meniscus to pass from the top edge of mark E to the top edge of mark F. For polymer solutions containing small amounts of finely divided pigments, such as carbon black, it shall be necessary to view the top of the meniscus. Where large concentrations of pigments are involved, it shall be necessary to centrifuge the solution before proceeding.

The opening and closing of the tubes may be carried out conveniently by means of taps or clips on clean flexible tubing attached to the ends of the tubes, making sure that no fluff or other contaminant enters the tube.

The first flow shall not be taken into account for measuring the efflux time. Repeat the measurement of efflux time immediately, without emptying or recharging, until two successive efflux times agree to within 0,25 %. Take the mean of these two values as the efflux time.

If two successive determinations of the mean efflux time of the solvent differ by more than 0,4 s, clean the viscometer as specified in [Annex A](#).

The efflux time for any “new” solution, created by the addition of solvent to an existing solution held in the viscometer, shall be determined as a separate liquid, in accordance with this procedure.

## 9 Expression of results

### 9.1 Reduced viscosity and intrinsic viscosity

Results are preferably expressed as a reduced viscosity.

The reduced viscosity  $I$ , in the units  $10^{-3} \text{ m}^3/\text{kg}$ , i.e.  $\text{cm}^3/\text{g}$ , is calculated using [Formula \(3\)](#):

$$I = \frac{t - t_0}{t_0 c} \quad (3)$$

$t$  is the efflux time of the solution, in seconds;

$t_0$  is the efflux time of the solvent, in seconds, through the same viscometer;

$c$  is the concentration, expressed as  $10^3 \text{ kg}/\text{m}^3$ , i.e.  $\text{g}/\text{cm}^3$ .

The results can also be expressed as an intrinsic viscosity  $[\eta]$ , for example in order to compare copolymers of different average molecular masses for which it has been necessary to use different concentrations (see [6.2](#)).

The intrinsic viscosity shall be calculated from the values of inherent viscosity or reduced viscosity obtained for concentrations  $c_1, c_2, c_3 \dots$ , in the approximate ratio  $1 : 2 : 3 \dots$ , by a graphical method consisting of plotting the inherent-viscosity values or the reduced-viscosity values (on the ordinate axis) against the concentration (on the abscissa) and extrapolating the curve to zero concentration. The intrinsic viscosity is read off the ordinate axis.

It is recommended that the method of least squares be used for analysing the experimental values.

The intrinsic viscosity  $[\eta]$  can also be calculated from one value of the reduced viscosity, for instance by using [Formula \(4\)](#):

$$[\eta] = \frac{l}{1 + k'cl} \quad (4)$$

where  $k'$  is an experimental constant, usually between 0,2 and 0,3, which must be determined previously by measuring the reduced viscosity at two different concentrations and applying [Formula \(5\)](#):

$$k' = \frac{l_2 - l_1}{l_1 l_2 (c_2 - c_1)} \quad (5)$$

In the calculation of  $k'$ , it should be preferable to use several concentrations and plot  $l$  against  $c$ , drawing a straight line through the points and selecting two positions on this line to give values for substitution in the formula for  $k'$ .

## 9.2 K-value

The K-value can be calculated from the relationship shown as [Formula \(6\)](#):

$$\text{K-value} = 1\,000\,k \quad (6)$$

where  $k$  is defined by the formulae given in [3.2.6](#).

## 10 Test report

The test report shall contain the following particulars:

- a) a reference to this document, i.e. ISO 1628-1:2021, and the particular standard for the polymer tested, if one exists;
- b) all details necessary for identification of the material tested, including type, source and manufacturer's code number;
- c) the concentration of material in the solution used, a description of the solvent and details of the preparation of the solution;
- d) details of the viscometer used;
- e) the temperature of the test;
- f) the test results;
- g) the date of the test.

## Annex A (normative)

### Cleaning of apparatus

It is essential that all apparatus coming into contact with the liquid under test is scrupulously clean. Any impurities, such as dust, traces of liquid or filaments in the viscometer, will cause false results to be obtained.

Before the test, clean the viscometer and all other apparatus used (glass vessels, pipettes, sintered-glass filters, rubber tubing, etc.). A suitable detergent may be adequate. Aqua regia (3 volumes concentrated hydrochloric acid and 1 volume concentrated nitric acid) may be required to remove inorganic residues from the glassware, and a suitable solvent may be required to remove oil and grease. Following this, dry the glass apparatus and then clean it with specially prepared chromic acid solution. Leave this solution in contact with the glassware overnight at a minimum temperature of 20 °C. For more active cleaning, warm the chromic acid gently on a water bath.

Remove the chromic acid and rinse at least five times with distilled or deionized water. Dry in an electric oven at a temperature no higher than 100 °C or rinse at least five times with acetone that has been distilled, dried and filtered, drying the apparatus with a slow stream of filtered dry air or, preferably, with a vacuum line.

Between successive determinations of the efflux times of samples of a similar nature, the viscometer shall be cleaned by draining and thoroughly rinsing with a suitable volatile solvent that has been distilled and filtered. Dry the apparatus with a slow stream of filtered dry air, with a vacuum line, or in an electric oven at a temperature no higher than 100 °C. The effectiveness of the cleaning can be checked by establishing that the efflux times with a given solvent and viscometer remain constant.

If the next solution to be measured is of a polymer of the same type and of similar viscosity, it is permissible to drain the viscometer, wash it with the next solution to be measured and then fill it with a further quantity of this solution.

It is recommended that viscometers used for silicone fluids and fluorocarbons be reserved exclusively for use with these fluids and that these viscometers be subject to calibration checks at frequent intervals. Great care shall be taken to ensure that these fluids do not contaminate other apparatus, either directly or indirectly.

**WARNING — Particular care should be taken when using aqua regia and chromic acid. Chromic acid is toxic. Appropriate action should also be taken to ensure the safe disposal of these acids. Goggles and protective gloves should be worn. Any splashes should be washed off the skin immediately with plenty of cold water. Inhalation of the vapours should be avoided.**



## Annex B (informative)

### Notes on sources of error

#### B.1 General

Guidance is given in this document on the determination of the viscometric properties of polymers in dilute solution as defined in [Clause 3](#). The measurement of these properties can usually be carried out with better reproducibility than that attained in absolute measurements of viscosity since many of the instrumental errors are approximately the same for both solvent and solution, and are effectively cancelled.

#### B.2 Principle of measurements

The relative viscosity and the other parameters defined in [Clause 3](#) are calculated from the efflux times of solution and solvent. The liquid flows, under the force of gravity, through the capillary of a suspended-level Ubbelohde viscometer. The efflux times are taken to be proportional to the viscosity/density ratio of the fluids (see [Clause 4](#)). This is equivalent to stating that the kinetic energy and other errors are negligible and that the density of the solvent differs negligibly from the density of the solutions.

#### B.3 Sources of error

The most important sources of error in capillary viscometry are related to

- a) surface tension,
- b) capillary end effects,
- c) drainage effects,
- d) viscous heat effects,
- e) deviation of the viscometer from the vertical,
- f) hydrostatic head variations,
- g) losses by evaporation,
- h) errors in the measurement of the concentration and efflux time,
- i) shear effects,
- j) errors in temperature stability and measurement,
- k) kinetic energy.

Fortunately, most of these effects can be considered negligible for the proposed procedures. Errors due to surface tension, end effects and drainage effects are quite small in tests with organic solvents in the Ubbelohde viscometer, when relative measurements of viscosity are concerned<sup>[2],[3]</sup>. Viscous heat effects are negligible when the capillary viscometer is operated by gravity. Errors due to deviation from the vertical and variations in the hydrostatic head are usually very small with this type of viscometer.

Solvent losses by evaporation and concentration errors depend on the particular test procedure and have to be taken into account.

The solvent efflux time should preferably be at least 70 s in order to measure it reproducibly, but it should not be longer than about 200 s in order to avoid long efflux times for the corresponding solutions.

The effect of shear rate can be serious, since polymer solutions are often non-Newtonian<sup>[4],[5]</sup>. Strictly speaking, the measurements should be carried out at very low shear rates, but in the usual procedures the shear rate is as high as 1 000 s<sup>-1</sup> or more. Fortunately, it can be shown<sup>[6],[7],[8]</sup> that shear rate effects are very small unless the molar mass of the polymer is higher than 10<sup>6</sup> g/mol, which seldom happens with commercial polymers. Furthermore, it is impractical to take account of shear rate effects for the purposes of international standardization, and a better approach is to define the tolerance of the viscometer dimensions in such a way that the shear rate is closely reproducible in different laboratories testing the same polymer sample.

It can be concluded that the most important source of error in the measurements is the kinetic-energy term. Its value may be considerable. For example, it is approximately 15 % for chloroform in a standard Ubbelohde viscometer having a capillary diameter of 0,58 mm. The resultant error in the reduced viscosity will be of the order of 30 % and, for special work outside the scope of this document, it might be appropriate to include a kinetic-energy correction.

#### B.4 Choice of viscometers

Since it is impractical to introduce a kinetic-energy correction into international standardization, it is necessary to choose the viscometer in such a way that

- a) either the kinetic-energy term is negligible,
- b) or it is constant and reproducible in different laboratories.

It can be shown that the second condition cannot be realized easily. In fact, the maximum fractional hydrostatic pressure  $X$  spent in kinetic energy is given approximately by [Formula \(B.1\)](#)

$$X = \frac{R^4 h g}{64 L^2 \nu^2} \tag{B.1}$$

where

- $R$  is the radius of the capillary;
- $h$  is the hydrostatic head;
- $g$  is the acceleration due to gravity;
- $L$  is the length of the capillary;
- $\nu$  is the viscosity/density ratio.

It is important to note in [Formula \(B.1\)](#) that the efflux time and the reservoir volume by themselves do not influence the value of  $X$ .

For standard glass capillaries with diameters between 0,3 mm and 1,0 mm, the tolerance limits for the diameter<sup>[9],[10]</sup> are usually  $\pm 0,02$  mm, corresponding to approximately  $\pm 30$  % and  $\pm 8$  %, respectively, of the value of  $X$ , whereas the mean hydrostatic head  $h$  is 120 mm  $\pm$  10 mm and the capillary length  $L$  is 90 mm  $\pm$  9 mm, corresponding to approximately  $\pm 30$  % of the value of  $X$ . The conclusion is that, unless the normal tolerances on standard capillaries are severely restricted, the kinetic-energy term cannot be made reproducible. It is therefore necessary to choose viscometers which minimize it.

In this document, the maximum permitted value of  $X$  is fixed at 0,03 (approximately 4 % to 6 % of the reduced viscosity).

From [Formula \(B.1\)](#), it can be seen that, at fixed values of  $h$  and  $L$ , the critical parameter which defines the magnitude of  $X$  is the ratio  $R^2/\nu$ .

By inserting

$$h = 120 \text{ mm,}$$

$$L = 90 \text{ mm}$$

and

$$X < 0,03$$

in [Formula \(B.1\)](#), a relationship between the maximum capillary radius to be used and the value of  $\nu$  is obtained as shown in [Formula \(B.2\)](#):

$$R^2 < 0,111\nu \quad (\text{B.2})$$

or, for the diameter,

$$D^2 < 0,444\nu \quad (\text{B.3})$$

where  $R$  and  $D$  are in mm and  $\nu$  is in  $\text{mm}^2 \cdot \text{s}^{-1}$ .

It will be noted that [Formula \(B.3\)](#) is dependent on the particular values ascribed to the mean hydrostatic head and the capillary length. These will vary between various designs of viscometer and, in particular, are slightly different for the Ubbelohde and DIN Ubbelohde versions.

[Formula \(B.3\)](#) permits calculation of the maximum theoretical diameter that could be used for a solvent whose viscosity/density ratio  $\nu$  is known at the temperature of measurement. It follows that, in order to determine the properties of polymers described in this document, the viscosity/density ratio for the solvent chosen must be known. [Table B.1](#) gives values at 25 °C for several of the established solvents for polymers, together with the calculated theoretical maximum capillary diameter for the Ubbelohde viscometer.

[Formula \(B.3\)](#) has also been used to select the recommended sizes of Ubbelohde and DIN Ubbelohde viscometers given in [Table 1](#). Other appropriate series of viscometers and sizes can be identified by substituting the relevant values into [Formula \(B.1\)](#).

**Table B.1 — Examples of viscosity/density ratios for established polymer solvents, and the corresponding maximum theoretical capillary diameters**

Solvent	Viscosity/density ratio at 25 °C	Maximum theoretical capillary diameter from <a href="#">Formula (B.3)</a>
	$\text{mm}^2 \cdot \text{s}^{-1}$	mm
Cyclohexanone	2,10	0,97
Dichloromethane	0,33	0,38
<i>m</i> -Cresol (meta-cresol)	13,10	2,41
Trichloromethane	0,36	0,40

## Bibliography

- [1] FIKENTSCHER H., *Cellulosechemie*, **13**, pp. 58-64 (1932)
- [2] ONYON P.F., in *Techniques of polymer characterisation*, ed. by ALLEN P.W., Butterworths, London, 1959
- [3] CRAGG L.H., VAN OENE H., *Can. J. Chem.*, **39**, 203 (1961)
- [4] PASSAGLIA E., YOUNG J.T., WEGEMER N.J., *J. Polymer Sci.*, **47**, 333 (1960)
- [5] LOHMANDER U., *Makromol. Chem.* **72**, 159 (1964)
- [6] KRIGBAUM W.R., FLORY P.J., *J. Polymer Sci.*, **11**, 37 (1953)
- [7] CRAGG L.H., STONES R.H., DUMITRU T.E., *J. Polymer Sci.*, **13**, 167 (1954)
- [8] MERRIL E.W., MICKLEY H.S., RAM A., PERKINSON G. *Trans. Soc. Rheol.*, **5**, 237 (1961) and **6**, 119 (1962)
- [9] ASTM D 446, *Standard Specifications and Operating Instructions for Glass Capillary Kinematic Viscometers*
- [10] BS 188, *Methods for determination of the viscosity of liquids*



